


# CASE STUDY


Kera Trial Fitting



**Base Curve 6.40**  
0.4mm flatter than ideal. Excessive pressure on cone.

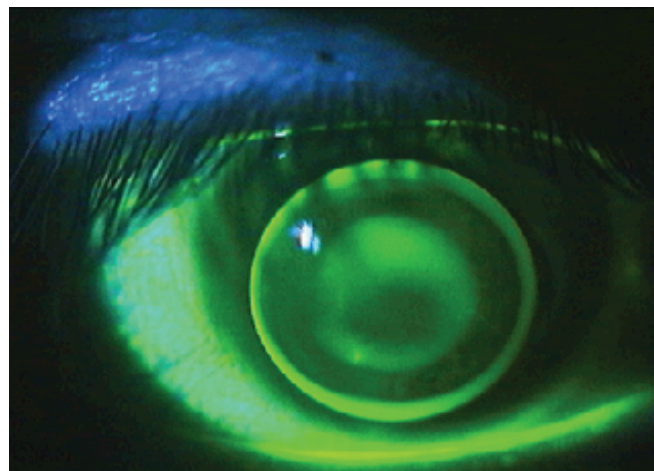

**Base Curve 6.20**  
0.2mm flatter than ideal.

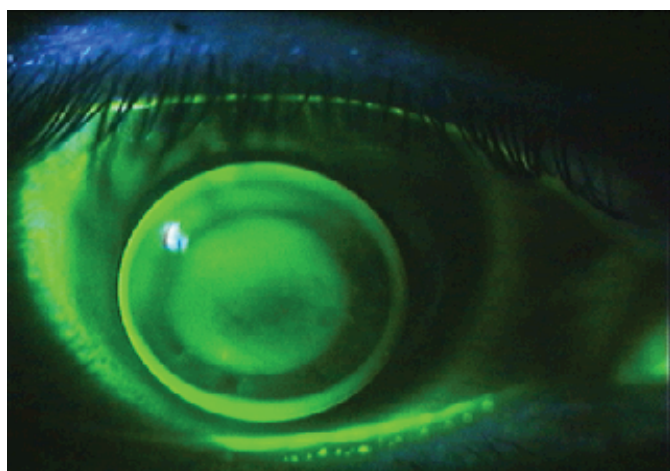

**Base Curve 6.00**  
Ideal fit for a trial lens.

Support is distributed over the cone and the periphery. Only slight pressure on the cone.